NANJING N.E. ORIENTAL IMPORT.& EXPORT. CO., LTD
702 FLOOR, B4 BUILDING, NO.118, RUANJIAN ROAD, YUHUATAI DISTRICT, NANJING

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description	:	(A) Surgical mask (Claimed Type IIR)
Buyer	:	MD FONSCARE
Composition	:	(A)55%Non-woven 25%melt-blown 10%bridge 10%earloop
Sample Color	:	(A)Blue
Style No.	:	MD FONSCARE MD-319R
Manufacturer	:	Jiangsu jinshaxiang technology Co., Ltd
Supplier	:	NANJING N.E. ORIENTAL IMPORT.& EXPORT. CO.,LTD
Country of Destination	:	France
Test Performed	:	Selected test(s) as requested by applicant
Sample Receiving Date	:	Sep 08, 2020
Testing Period	:	Sep 09, 2020 - Sep 21, 2020
Test Result(s)	:	Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Comment:

EN 14683:2019+AC:2019 Medical Face Masks-Requirements and Test Methods **Clause 5.2 Performance Requirement**	(A)
Clause 5.2.2 Bacterial filtration efficiency (BFE)	M
Clause 5.2.3 Breathability	M
Clause 5.2.4 Splash Resistance	M
Clause 5.2.5 Microbial Cleanliness	M
Clause 5.2.6 Biocompatibility	EXCLUDED

Remark: M=Meet EN 14683:2019+AC:2019 Performance Requirement (Type IIR)

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)

Dongjing Liu / Hailian Xuan (Authorized Signatory)

3rd Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Test Result

EN 14683:2019+AC:2019 Medical Face Masks-Requirements and Test Methods

Clause 5.2 Performance Requirement

Clause 5.2.2 Bacterial Filtration Efficiency (BFE)
(EN 14683:2019+AC:2019 Annex B)

Sample: A

Test Side	:	Inside
Test Area	:	Approximately 60 cm^2
Flow Rate	:	28.3 L/min
Pre-Conditioning	:	Minimum of 4 hours at 21±5°C and 85±5% R.H.
Dimensions of test specimen	:	~174mm x 157mm
Positive Control Average	:	2156 CFU
Negative Monitor Count	:	< 1 CFU
Mean Particle Size	:	3.0 ±0.3μm
Test bacteria	:	Staphylococcus aureus ATCC 6538

Test Item	Specimen No.	Result
Bacterial Filtration Efficiency (BFE), %	1	99.6
	2	99.9
	3	99.7
	4	99.9
	5	99.9

Remark:
1) Performance Requirement: Type I≥95%, Type II≥98%, Type IIR ≥98%
2) The number of specimens that shall be tested is minimum 5, but can be greater and shall be increased if necessary to allow for an AQL(Acceptable Quality Level) of 4%.

3rd Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 5.2.3 Breathability
(EN 14683 :2019+AC:2019 Annex C)

Sample: A
Test Side : Randomly test in different location (1 around and 4 away from the centric point) on each of the 5 masks
Pre-Conditioning : Minimum of 4 hours at 21±5°C and 85±5% R.H.
Test Area : 4.9 cm^2
Flow Rate : 8 l/min

Specimen No.	Test Area No.	Different Pressure for each tested area (Pa/cm^2)	The average value for each test specimen (Pa/cm^2)
1	1-1	38.2	38
	1-2	35.2	
	1-3	38.0	
	1-4	36.9	
	1-5	39.2	
2	2-1	39.5	38
	2-2	38.5	
	2-3	38.8	
	2-4	38.3	
	2-5	36.6	
3	3-1	34.2	37
	3-2	35.8	
	3-3	36.3	
	3-4	39.7	
	3-5	38.5	
4	4-1	29.7	33
	4-2	32.1	
	4-3	31.6	
	4-4	36.1	
	4-5	36.3	
5	5-1	30.4	30
	5-2	27.4	
	5-3	26.3	
	5-4	35.7	
	5-5	30.4	

Remark:
1) Performance Requirement: Type I<40 Pa/cm^2, Type II<40 Pa/cm^2, Type IIR<60 Pa/cm^2
2) The number of specimens that shall be tested is minimum 5, but can be greater and shall be increased if necessary to allow for an AQL(Acceptable Quality Level) of 4%.

3rd Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 5.2.4 Splash Resistance
(ISO 22609 :2004)

Sample: A
Test Blood Pressure : 16.0kPa
Pre-Conditioning : Minimum of 4 hours at 21±5°C and 85±5% R.H.
Distance of the mask to the tip of cannula : 300±10mm

Test Specimen#	Penetration on inside surface	Conclusion	Test Specimen#	Penetration on inside surface	Conclusion
1	None Seen	Pass	17	None Seen	Pass
2	None Seen	Pass	18	None Seen	Pass
3	None Seen	Pass	19	None Seen	Pass
4	None Seen	Pass	20	None Seen	Pass
5	None Seen	Pass	21	None Seen	Pass
6	None Seen	Pass	22	None Seen	Pass
7	Seen	Fail	23	None Seen	Pass
8	None Seen	Pass	24	None Seen	Pass
9	None Seen	Pass	25	None Seen	Pass
10	None Seen	Pass	26	None Seen	Pass
11	None Seen	Pass	27	Seen	Fail
12	None Seen	Pass	28	None Seen	Pass
13	Seen	Fail	29	None Seen	Pass
14	None Seen	Pass	30	None Seen	Pass
15	None Seen	Pass	31	None Seen	Pass
16	None Seen	Pass	32	None Seen	Pass
Number of Pass:		29			
Overall result:		Acceptable			

Remark:
1) Performance Requirement Type I: N/A, Type II: N/A, Type IIR: ≥16.0kPa
2) Test was conducted within 60s after removal from conditioning chamber.
3) An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show pass results.

Clause 5.2.5 Microbial Cleanliness
(EN 14683:2019+AC:2019 Annex D and EN ISO 11737-1:2018)

Sample Number	Mask Weight(g)	Total Bioburden, (cfu/mask)	Total Bioburden, (cfu/g)
1#	3.61	3	0.83
2#	3.64	6	1.65
3#	3.63	3	0.83
4#	3.66	6	1.64
5#	3.67	3	0.82

Remark: Performance Requirement: Type I≤30 CFU/g, Type II≤30 CFU/g, Type IIR≤30 CFU/g

3rd Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Sample Photo

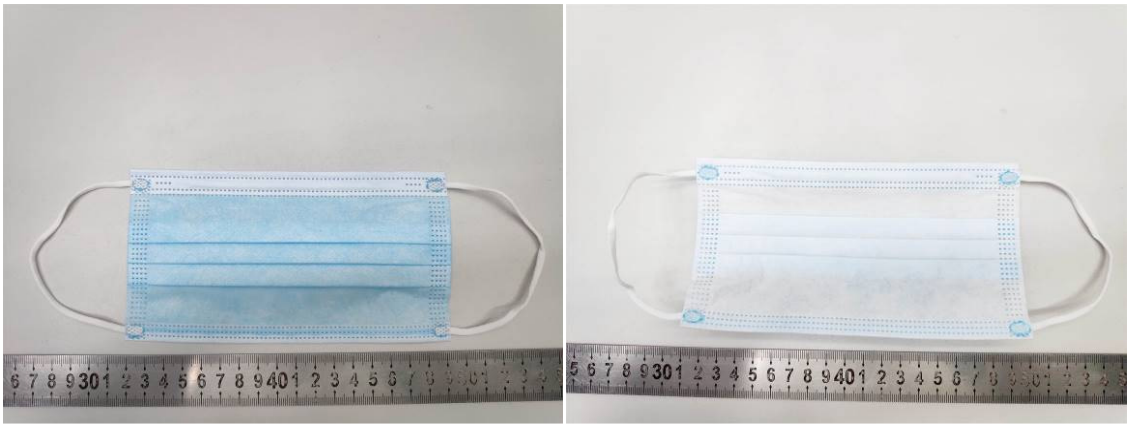

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report

SGS-CSTC Standards Technical Services (Shanghai) Co.,Ltd. Testing Center
检验检测专用章 Inspection & Testing Services
3rd Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com